



## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Sirolan Laserscan Micron Test Report

Toft Alpacas/Rob & Shirley Bettinson  
Toft Manor, Dunchurch  
Nr Rugby CV22 6NR UK

09/20/13

Test No: 471079


#### Animal and Sample Description

**Animal Name:** Ikrit (288)  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Dark Brown

**Animal ID:** 4611  
**Sample Location:** Side  
**Sample Date:** 05/13/13  
**Age:** 08/19/11

#### Laboratory Data

**Mean Fiber Diameter:** 20.0 microns  
**Standard Deviation:** 3.5 microns  
**Coefficient of Variation:** 17.6 %  
**Fibers Greater Than 30 microns:** 1.0 %

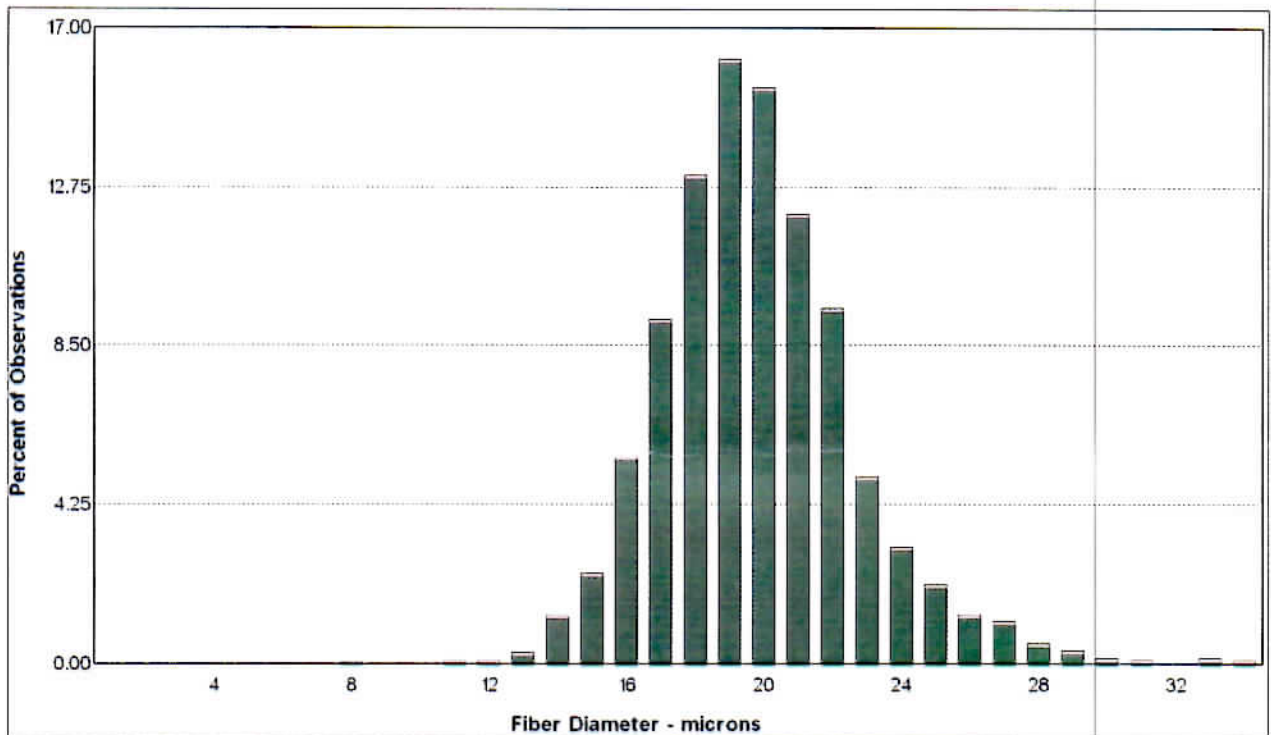

This Test Performed According to I.W.T.O Method 12