



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Toft Alpacas/Rob & Shirley Bettinson
Toft Manor, Dunchurch
Nr Rugby CV22 6NR UK

09/20/13


Test No: 471079

Animal and Sample Description

Animal Name: Ikrit (288)	Animal ID: 4611
Breed: Alpaca(Huacaya)	Sample Location: Side
Sex: Male	Sample Date: 05/13/13
Color: Dark Brown	Age: 08/19/11

Laboratory Data

Mean Fiber Diameter:	20.0 microns
Standard Deviation:	3.5 microns
Coefficient of Variation:	17.6 %
Fibers Greater Than 30 microns:	1.0 %

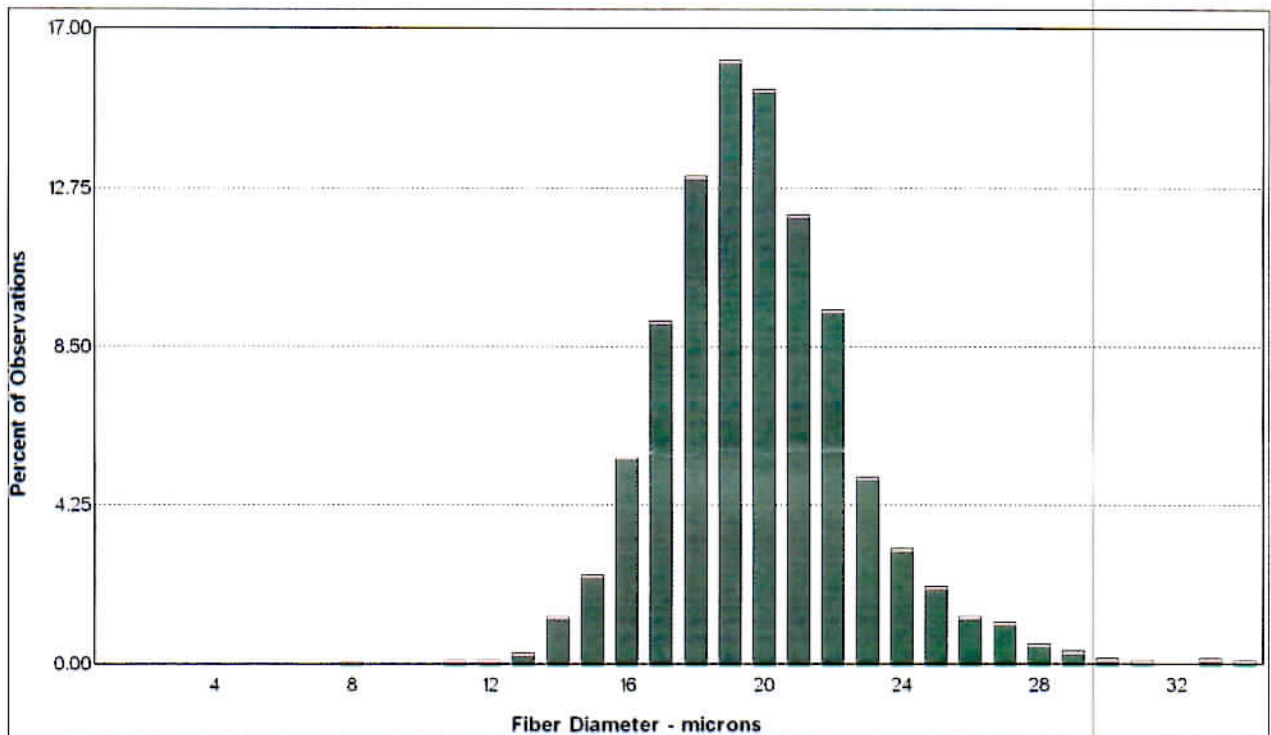

This Test Performed According to I.W.T.O Method 12